FREEDOM DIAGNOSTICS

Certificate of Analysis

FreedomDiagnosticsTesting.com
Admin@FreedomDiagnostics.net



Client:	Modern Aminos
Accession #:	2611044320
Search Code:	Mode2611044320
Received:	11/4/2026
Reported:	11/8/2026
Lot:	BX-C-K5J8

Sample Summary


Product:	**9-ME-BC 15mg**	Net Content:	**14.31 mg**
Identity:	**Confirmed**		
Appearance:	**White Capsule**		

Analytical Results


Test	Result
Identity (LC-MS)	**9-ME-BC**
Net Content	**14.31 mg**

Method: HPLC with UV detection coupled with mass spectrometry (LC-MS).

Chromatogram

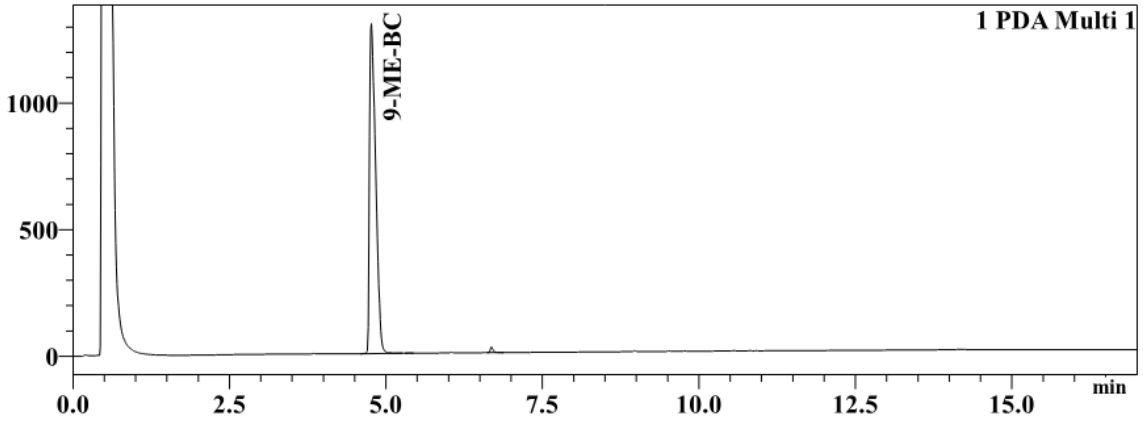

Mass Confirmation

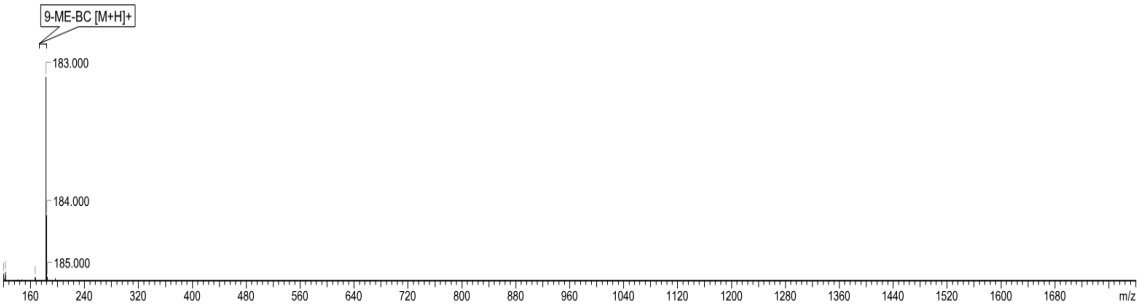

Alex Johnson

Principal Chemist
CoA Template v3.1

FreedomDiagnosticsTesting.com
Admin@FreedomDiagnostics.net
Proudly Owned and Operated in the USA

The peptide purity analysis reported here was conducted using LCMS/MS under standard laboratory conditions. This analysis is for informational purposes only and is specific to the sample(s) provided. The peptides tested are for research use only and are not approved for human, veterinary, diagnostic, therapeutic, or clinical use. Results should be interpreted by qualified professionals. Accuracy may be influenced by sample integrity, handling, and other experimental variables.

Customer:
Modern Aminos

EA Sample ID: 26EA1104-026
Sample Name: 9-Me-BC
Sample Type: Powder Capsule
Batch/Lot: BX-C-K5J8

Date Received:
11/04/2026
Date Completed:
11/12/2026

ETHOS ANALYTICS

CERTIFICATE OF ANALYSIS

Summary of Results

Analysis Type	Method	Date Tested	Status
9-me-BC	HPLC	11/12/2026	Pass



Serving Size: N/A

Label Claim Profile

Analyte	Result	Specification	LOQ (%)
9-Methyl-β-carboline (9-me-BC)	15.39mg/capsule	15mg/capsule	0.01

Identity of the analyte was confirmed by retention time concordance with a certified reference standard, per USP <621>.

NOTES:

LOD = LIMIT OF DETECTION; LOQ = LIMIT OF QUANTIFICATION

ETHOS ANALYTICS
Ethos Analytics Laboratory
3020 E Camelback Rd STE 397
Phoenix, AZ 85016
Info@Ethosanalytics.io
www.Ethosanalytics.io
Lic #: 000026LRCND60176649
ISO/IEC 17025 Acc #: 117798

Noel Samsum
Laboratory Director
12-Nov-2026

The sample analyzed was inspected and is free from visual mold, mildew, and foreign matter. The testing procedures, equipment calibration, and maintenance are all in accordance with ISO/IEC 17025:2017 standards. The presented report is only applicable to the sample specified above and may not be applied to any similar or identical products. Reports are prohibited from being reproduced with alterations of any kind.